

(12) INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(19) World Intellectual Property
Organization
International Bureau



(43) International Publication Date
18 March 2004 (18.03.2004)

PCT

(10) International Publication Number
WO 2004/023153 A1

(51) International Patent Classification⁷: G01R 33/28

(21) International Application Number:
PCT/IB2003/003785

(22) International Filing Date: 25 August 2003 (25.08.2003)

(25) Filing Language: English

(26) Publication Language: English

(30) Priority Data:
102 40 960.9 5 September 2002 (05.09.2002) DE

(71) Applicant (for DE only): PHILIPS INTELLECTUAL
PROPERTY & STANDARDS GMBH [DE/DE]; Stein-
damm 94, 20099 Hamburg (DE).

(71) Applicant (for AE, AG, AL, AM, AT, AU, AZ, BA, BB, BE,
BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CY, CZ, DK,
DM, DZ, EC, EE, ES, FI, FR, GB, GD, GE, GH, GM, GR,
HR, HU, ID, IE, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC,
LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX,
MZ, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC, SD,
SE, SG, SK, SL, SY, SZ, TJ, TM, TN, TR, TT, TZ, UA, UG,
UZ, VC, VN, YU, ZA, ZM, ZW only): KONINKLIJKE
PHILIPS ELECTRONICS N.V. [NL/NL]; Groenewoud-
seweg 1, NL-5621 BA Eindhoven (NL).

(72) Inventors; and

(75) Inventors/Applicants (for US only): SCHULZ, Volkmar

[DE/DE]; c/o Philips Intellectual Property & Standards
GmbH, Weissshausstr. 2, 52066 Aachen (DE). GLEICH,
Bernhard [DE/DE]; c/o Philips Intellectual Property &
Standards GmbH, Weissshausstr. 2, 52066 Aachen (DE).

(74) Agent: MEYER, Michael; Philips Intellectual Property &
Standards GmbH, Weissshausstr. 2, 52066 Aachen (DE).

(81) Designated States (national): AE, AG, AL, AM, AT, AU,
AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU,
CZ, DE, DK, DM, DZ, EC, EE, ES, FI, GB, GD, GE, GH,
GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC,
LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW,
MX, MZ, NI, NO, NZ, OM, PG, PH, PL, PT, RO, RU, SC,
SD, SE, SG, SK, SL, SY, TJ, TM, TN, TR, TT, TZ, UA,
UG, US, UZ, VC, VN, YU, ZA, ZM, ZW.


(84) Designated States (regional): ARIPO patent (GH, GM,
KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZM, ZW),
Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM),
European patent (AT, BE, BG, CH, CY, CZ, DE, DK, EE,
ES, FI, FR, GB, GR, HU, IE, IT, LU, MC, NL, PT, RO,
SE, SI, SK, TR), OAPI patent (BF, BJ, CF, CG, CI, CM,
GA, GN, GQ, GW, ML, MR, NE, SN, TD, TG).

Published:

— with international search report

For two-letter codes and other abbreviations, refer to the "Guid-
ance Notes on Codes and Abbreviations" appearing at the begin-
ning of each regular issue of the PCT Gazette.

(54) Title: CATHETER FOR USE IN MR IMAGING

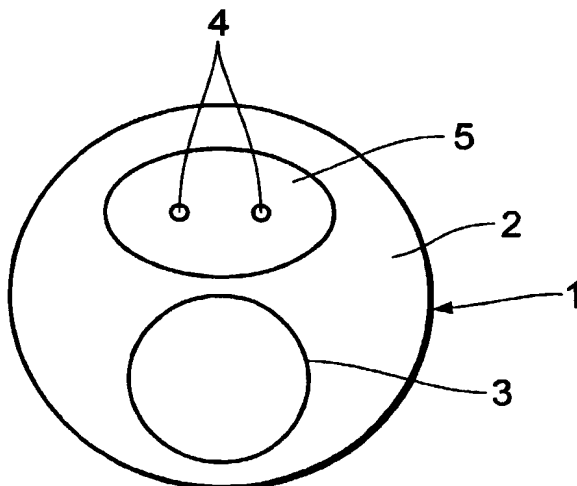

(57) Abstract: The invention relates to a catheter which is suitable in particular for use in MR imaging. In order to avoid undesirable heating of the tissue surrounding the catheter by the MR excitation field, the catheter in accordance with the invention comprises: a catheter sleeve (2), a hollow guide channel or lumen (3) within the catheter sleeve (2) for the introduction of a medical instrument, and two electrical conductors (4) which are enclosed by a cable sheath (5) of a dielectric material and serve to transmit RF signals within the catheter envelope (2), the dielectric material having a relative permittivity (ϵ_r) smaller than 4, the diameter of the electrical conductors (4) being between 5 and 50 μm , notably between 10 and 30 μm , and the distance between the electrical conductors (4) being smaller than 300 μm , in particular smaller than 200 μm .

WO 2004/023153 A1

CATHETER FOR USE IN MR IMAGING

The invention relates to a catheter which is suitable especially for use in magnetic resonance imaging (MR imaging), as well as to an MR device for forming MR images of an object to be examined, in particular for intravascular interventional MR imaging.

5

A catheter for use in MR imaging is known from US 5,792,055. The catheter therein is formed by a coaxial cable which serves as an antenna. As a result, the catheter can be localized during an intravascular intervention so as to be imaged in MR images. It is a drawback, however, that in response to the RF excitation of the spins the tissue surrounding the coaxial cable is heated due to the standing waves arising around the cable (common mode resonance). This could damage the surrounding tissue.

15 Therefore, it is an object of the invention to provide a catheter, in particular for use in MR devices, as well as a corresponding MR device in which the described undesirable heating of the tissue surrounding the catheter is avoided.

This object is achieved by means of a catheter as disclosed in claim 1 which comprises:

- 20 - a catheter sleeve (2),
 - a hollow guide channel or lumen (3) within the catheter sleeve (2) for receiving a medical instrument, and
 - two electrical conductors (4) which are enclosed by a cable sheath (5) of a dielectric material and serve for the transmission of RF signals within the catheter sleeve (2),
25 the dielectric material having a relative permittivity (ϵ_r) which is smaller than 4, the diameter of the electrical conductors (4) being between 5 and 50 μm , notably between 10 and 30 μm , and the distance between the electrical conductors (4) being smaller than 300 μm , in particular smaller than 200 μm .

The object of the invention is also achieved by means of an MR device as claimed in claim 6 which includes:

- a main field magnet system (16) for generating a homogeneous, steady main magnetic field,

5 - a gradient coil system (17, 18, 19) for generating magnetic gradient fields,

- an RF coil system (14) for exciting an examination zone,

- a receiving coil system (14, 12) for receiving MR signals from the examination zone,

10 - a catheter (1) as claimed in claim 1 for introducing a medical instrument into the object (10) to be examined, notably comprising an active coil (4, 5) which is arranged on or in the catheter (1) for the purpose of catheter localization, local excitation of the examination zone and/or local reception of MR signals, and

- a control unit (23) for controlling the MR device.

The invention is based on the idea to configure the catheter in such a manner
15 that no resonance can occur up to the MR frequency used. To this end, in accordance with the invention there is provided a cable which comprises two electrical conductors which are enclosed by a cable sheath of a dielectric material, the cable being constructed in such a manner that it has a low shortening factor. In this context the shortening factor is defined as the square root of the product of the relative permittivity (ϵ_r) and the relative
20 permeability (μ_r), the shortening of the wavelength used resulting from the fact that the electromagnetic wave does not propagate in vacuum but in a medium having a relative permittivity and/or relative permeability larger than 1. When a shortening factor is chosen in this manner, the common mode resonance of the cable is shifted beyond the MR frequency.

Moreover, in accordance with the invention it is arranged to utilize a
25 miniaturized pair of cables where the individual conductors have only a small diameter and are situated at a small distance from one another. In order to achieve an as small as possible shortening factor also during the intervention, the diameters of the conductors should be as small as possible; however, they should not be too small, as otherwise large signal losses will occur. Therefore, the indicated orders of magnitude represent a suitable compromise.

30 Advantageous embodiments of the catheter in accordance with the invention are disclosed in the dependent claims. In a preferred embodiment the dielectric material has a relative permittivity which is smaller than 2.3, notably smaller than 1.5. For example, polytetrafluoroethylene (PTFE), having a relative permittivity of approximately 2.3, could be used as the dielectric material.

Alternatively, in particular aerated synthetic materials are suitable for use as a dielectric material for the cable sheath, because the relative permittivity of such materials is nearly 1. An example in this respect is, for example, the material FP301040 or FP301020 (marketed by Good Fellow). Shortening factors as small as 1.2 can thus be achieved, the
5 choice of the suitable dielectric material also being dependent on the field strength of the main field magnets of the MR device used.

In conformity with a further embodiment of the invention, the two electrical conductors are also arranged to conduct a direct voltage for the voltage supply of a medical instrument arranged on or in the catheter. An example in this respect is an active coil in
10 conformity with a further embodiment which is arranged at the tip of the catheter and can act for catheter localization during an intervention or also for MR signal acquisition in its direct vicinity.

The invention can in principle be used in all MR devices in which especially intravascular interventions have to be carried out, in particular in MR devices with a field
15 strength of up to 2 Tesla, that is, for typical patient sizes; when only small catheter lengths are required, for example, in the case of small children, examinations can also be performed with greater field strengths. In a 1.5 Tesla system catheters can be used with a length of up to 1.6 m. The catheter in accordance with the invention thus constitutes an economical solution which can be readily implemented and whereby the undesirable heating of the tissue
20 surrounding the catheter by the excitation field for the spins is avoided.

The invention will be described in detail hereinafter with reference to the drawings. Therein:

25 Fig. 1 is a cross-sectional view of a catheter in accordance with the invention, and

Fig. 2 is a simplified representation of an MR device in accordance with the invention which is provided with a catheter of this kind.

30 Fig. 1 is a cross-sectional view of a catheter 1 in accordance with the invention. It consists of a catheter sleeve 2 which consists, for example, of a flexible synthetic material. Inside the catheter sleeve 2 there is formed a guide channel (lumen) 3 wherethrough one or more medical instruments can be introduced into the object to be

examined, for example, the body of a patient. Furthermore, inside the catheter sleeve 2 there is provided a cable sheath 5 in which two electrical conductors 4 extend substantially parallel to one another so that they are completely enclosed by the cable sheath 5. The cable sheath 5 consists of a dielectric material having a dielectric number (permittivity) ϵ_r , which is smaller than 4, preferably smaller than 2.3. The diameter of the electrical conductors 4 preferably is in the range of between 10 and 30 μm , for example, 15 μm , and the distance between the conductors 4 preferably is smaller than 200 μm , for example, 50 μm .

The described configuration results in a small shortening factor and the lowest resonance frequency of the cable is thus shifted to a range which does not correspond to the MR frequency used and which does not change due to the presence of the tissue. The shortening factor has an effect on the resonance frequency in a sense that the resonance frequency of an antenna is in principle inversely proportional to the shortening factor. The use of a small diameter for the electrical conductors ensures that the electromagnetic energy is preferably stored in the vicinity of the conductor and hence less energy can be dissipated in the proximity, so that heating of the proximity of the catheter is also avoided.

Two conductors are provided so as to transmit signals in the so-called differential mode. In addition, a direct voltage which does not interfere with the MR signal in the RF range can also be conducted.

A suitable dielectric material for the cable sheath 5 is, for example, polytetrafluoroethylene which has a relative permittivity of from approximately 2.2 to 2.3. Preferably, use is made of an aerated, spongy synthetic material, for example, FP301040 or FP301020 (as marketed by Good Fellow), because such materials have a relative permittivity near 1.

Fig. 2 is a diagrammatic representation of an MR device in accordance with the invention in which the catheter in accordance with the invention can be used. A patient is arranged on a patient table 11 in order to carry out an intravascular intervention. A catheter 1 in accordance with the invention has been introduced into a main artery of the patient 10 in order to perform a treatment on the coronary arteries; it has been advanced as far as the coronary arteries by a physician. At its end which is introduced into the patient 10 the catheter is provided with an image acquisition device 12 and a localization device 13. The image acquisition device 12 may be, for example, a microcoil which is capable of receiving MR signals from its vicinity after excitation by means of an external excitation coil 14, said MR signals providing image information on the vicinity of the microcoil 4. By way of example, the localization device 13 is constructed as a magnetic field sensor which co-

operates with a coil system 15 arranged underneath the patient 10. Using the signals emitted by the individual coils of the coil array 15, the position of the magnetic field sensor, and hence the position of the end zone of the catheter 1, can be determined on the basis of the signals received by the magnetic field sensor. The described image acquisition by means of the microcoil 12 and the localization by means of the magnetic field sensor 13 are known per se and, therefore, will not be elaborated herein.

The MR device also includes a main field magnet system 16 which comprises a plurality of main field magnets which generate a steady, uniform magnetic field in the longitudinal direction of the patient 10. In order to generate magnetic gradient fields there is provided a gradient coil system which comprises a plurality of gradient coils 17, 18, 19. Furthermore, an RF coil system 14 is provided so as to generate RF excitation pulses and to pick up MR signals from the excited examination zone.

For the processing of the signals received by the microcoil 12 or for the control of the microcoil 12 and the excitation coil 14 there is provided an image processing and control device 20 which converts the measured signals into image information which is applied to a data processing device 21. A position processing and control unit 22 is provided for the processing of the signals picked up by the magnetic field sensor 13 and for controlling the magnetic field sensor and the coil array 15, which unit 22 converts the measured signals into position data which is applied to the data processing device 21. The control of said coils and units is performed by a control unit 23. The evaluation and reproduction of said signals as well as the operation of such an MR device are also known per se and, therefore, will not be elaborated either.

The catheter in accordance with the invention, which can be manufactured simply and economically, effectively prevents the heating of the part of the tissue of the patient 10 which surrounds the catheter. The catheter can be used for various applications in MR imaging.

CLAIMS:

1. A catheter which is intended especially for use in MR imaging and which includes

- a catheter sleeve (2),
- a hollow guide channel or lumen (3) within the catheter sleeve (2) for

5 receiving a medical instrument, and

- two electrical conductors (4) which are enclosed by a cable sheath (5) of a dielectric material and serve for the transmission of RF signals within the catheter sleeve (2), the dielectric material having a relative permittivity (ϵ_r) smaller than 4, the diameter of the electrical conductors (4) being between 5 and 50 μm , notably between 10 and 30 μm , and the
10 distance between the electrical conductor (4) being smaller than 300 μm , in particular smaller than 200 μm .

2. A catheter as claimed in claim 1, characterized in that the dielectric material has a relative permittivity which is smaller than 2.3, notably smaller than 1.5.

15

3. A catheter as claimed in claim 1, characterized in that the dielectric material is an aerated synthetic material, notably FP301040 or FP301020 as marketed by Good Fellow.

4. A catheter as claimed in claim 1, characterized in that the two electrical

20 conductors (4) are also arranged to conduct a direct voltage to the voltage supply of a medical instrument arranged on or in the catheter (1).

5. A catheter as claimed in claim 1, characterized in that it includes means for catheter localization during an intervention, notably at least one active coil (4, 5) which is

25 arranged on or in the catheter (1).

6. An MR device for forming MR images of an object to be examined, intended especially for intravascular interventional MR imaging, which device includes:

- a main field magnet system (16) for generating a homogeneous steady main magnetic field,

- a gradient coil system (17, 18, 19) for generating magnetic gradient fields,

- an RF coil system (14) for the exciting an examination zone,

5 - a receiving coil system (14, 12) for receiving MR signals from the examination zone,

- a catheter (1) as claimed in claim 1 for introducing a medical instrument into the object (10) to be examined, notably comprising an active coil (4, 5) which is arranged on or in the catheter (1) for the purpose of catheter localization, local excitation of the

10 examination zone and/or local reception of MR signals, and

- a control unit (23) for controlling the MR device.

1/2


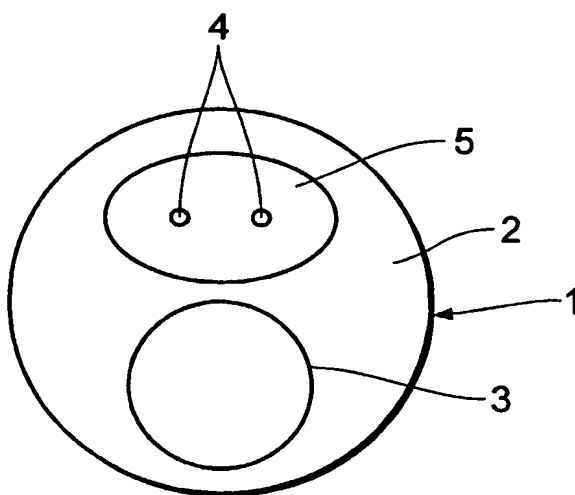


FIG.1

2/2

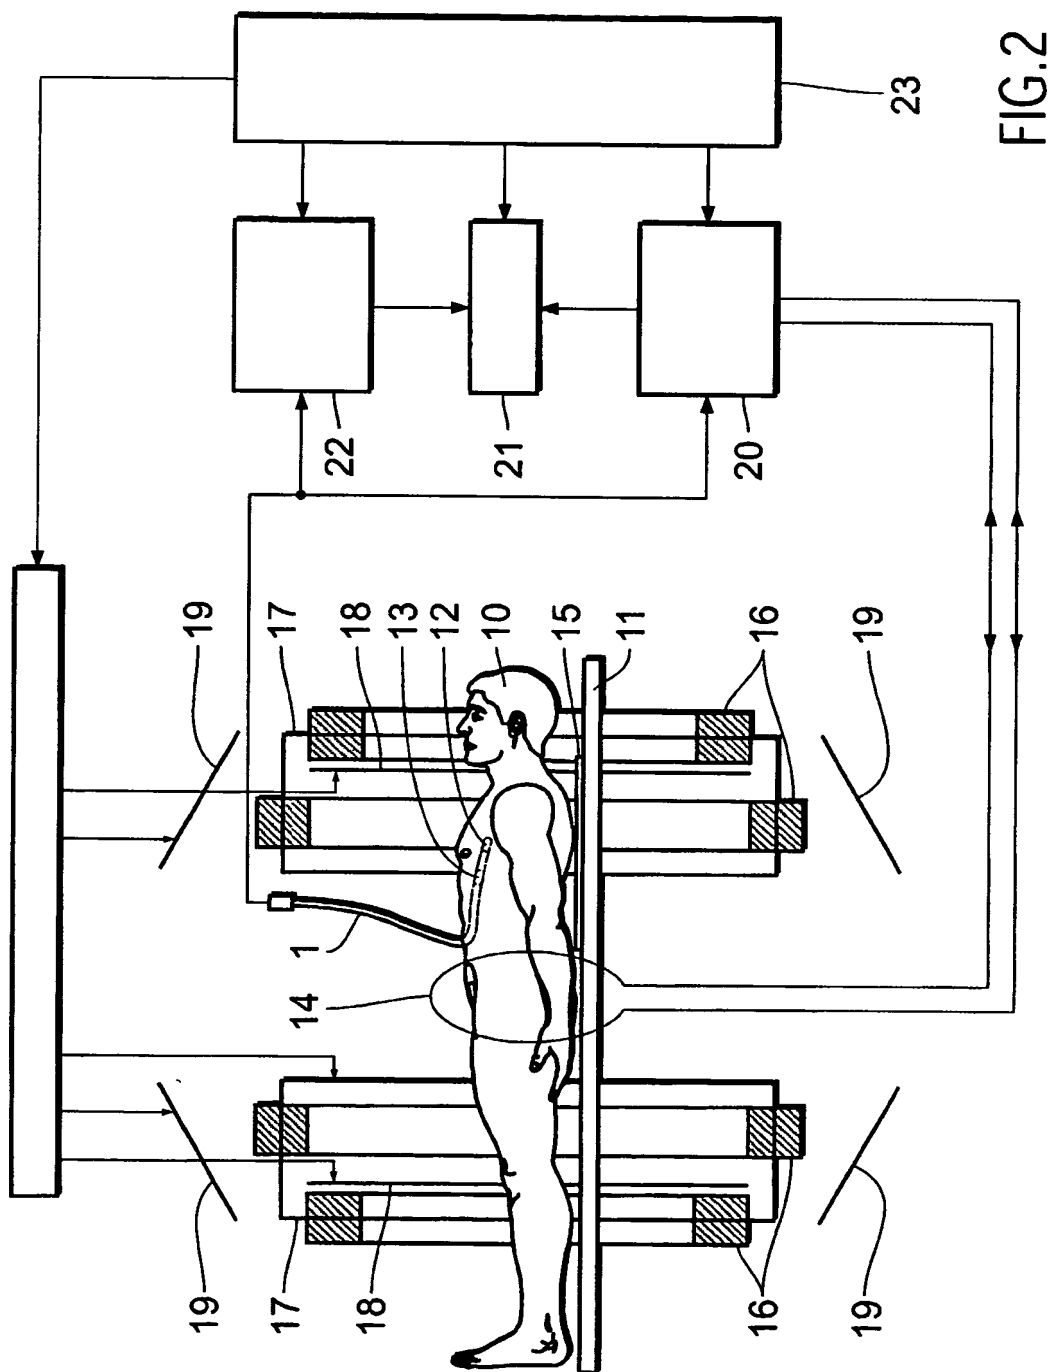

INTERNATIONAL SEARCH REPORT

Application No
PCT/IB 03/03785

A. CLASSIFICATION OF SUBJECT MATTER

IPC 7 G01R33/28

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 G01R

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal, INSPEC, EMBASE, BIOSIS, PAJ, WPI Data

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 2002/103430 A1 (GARIBALDI JEFFREY M ET AL) 1 August 2002 (2002-08-01) paragraph '0010! - paragraph '0015! paragraph '0035! - paragraph '0038!; figures 1-4	1,2,4-6
X	US 5 699 801 A (ATALAR ERGIN ET AL) 23 December 1997 (1997-12-23) column 7, line 30 -column 7, line 67 column 12, line 9 -column 12, line 34 column 15, line 1 -column 15, line 25; figures 2,3,22	1,2,4-6

☒ Further documents are listed in the continuation of box C.

☒ Patent family members are listed in annex.

* Special categories of cited documents :

- *A* document defining the general state of the art which is not considered to be of particular relevance
- *E* earlier document but published on or after the international filing date
- *L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- *O* document referring to an oral disclosure, use, exhibition or other means
- *P* document published prior to the international filing date but later than the priority date claimed

- *T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- *X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- *Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- *Z* document member of the same patent family

Date of the actual completion of the international search

5 November 2003

Date of mailing of the international search report

17/11/2003

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel. (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax: (+31-70) 340-3016

Authorized officer

Lersch, W

INTERNATIONAL SEARCH REPORT

International Application No
PCT/IB 03/03785

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT		
Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	<p>US 2002/007120 A1 (WHITE DAVID A ET AL) 17 January 2002 (2002-01-17) paragraph '0003! - paragraph '0006! paragraph '0117! - paragraph '0118! paragraph '0127! paragraph '0133! - paragraph '0134!; figures 11-13</p> <p style="text-align: center;">---</p>	1,4-6
X	<p>US 5 792 055 A (MCKINNON GRAEME C) 11 August 1998 (1998-08-11) cited in the application column 3, line 40 -column 4, line 24 column 5, line 28 -column 5, line 43; figures 1,4,5</p> <p style="text-align: center;">---</p>	1,2,5,6
A	<p>LADD M E ET AL: "Reduction of resonant RF heating in intravascular catheters using coaxial chokes" MAGNETIC RESONANCE IN MEDICINE, APRIL 2000, WILEY, USA, vol. 43, no. 4, pages 615-619, XP002260399 ISSN: 0740-3194 the whole document</p> <p style="text-align: center;">-----</p>	1-6

INTERNATIONAL SEARCH REPORT

Information on patent family members

Application No
PCT/IB 03/03785

Patent document cited in search report	Publication date	Patent family member(s)	Publication date
US 2002103430 A1	01-08-2002	WO 02074358 A2 US 2003195412 A1	26-09-2002 16-10-2003
US 5699801 A	23-12-1997	AU 6027196 A CA 2222742 A1 EP 0836414 A1 JP 2001525685 T WO 9638083 A1	18-12-1996 05-12-1996 22-04-1998 11-12-2001 05-12-1996
US 2002007120 A1	17-01-2002	US 6245020 B1 US 2002193690 A1 AU 2481199 A CA 2318771 A1 EP 1051109 A1 JP 2002500911 T WO 9937211 A1	12-06-2001 19-12-2002 09-08-1999 29-07-1999 15-11-2000 15-01-2002 29-07-1999
US 5792055 A	11-08-1998	EP 0673621 A1 AT 163525 T AU 685221 B2 AU 1490695 A CA 2141271 A1 DE 69408826 D1 DE 69408826 T2 DK 673621 T3 ES 2114626 T3 JP 2955484 B2 JP 7255694 A	27-09-1995 15-03-1998 15-01-1998 19-10-1995 19-09-1995 09-04-1998 23-07-1998 30-11-1998 01-06-1998 04-10-1999 09-10-1995

THIS PAGE BLANK (USPTO)